


Figure 1 ₩

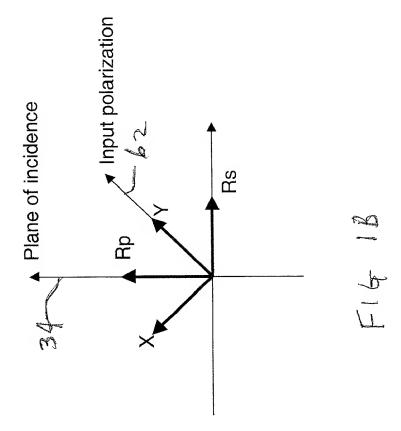

F 4.16

Polarizer Analyzer 44 Focusing optics 307 Reflected beam Sample Incident beam 100 / 147

65



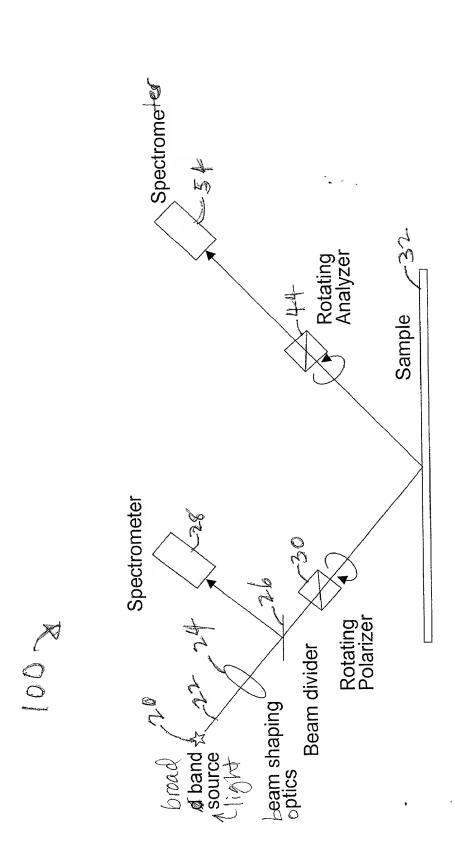


Figure 2. Ellipsometer or reflectometer with rotating polarizer and analyzer


正年3

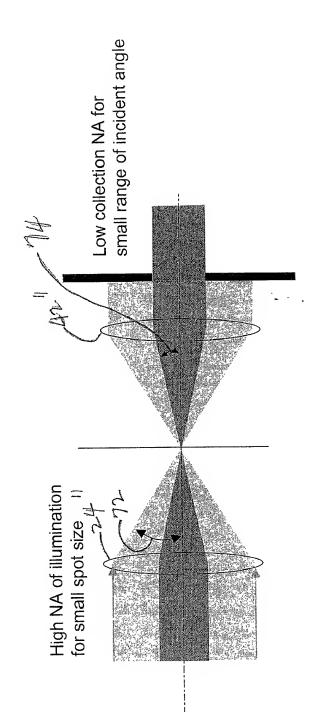


Eigure-2a: Asymmetric NA for illumination and collection. Shown in transmission mode, can be applied to reflection mode.

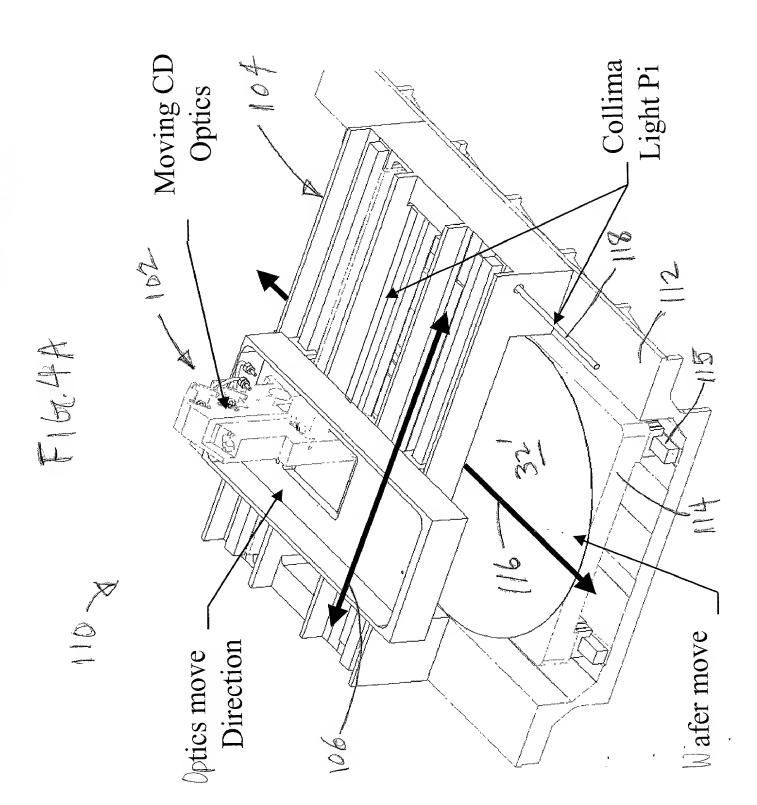

T & T

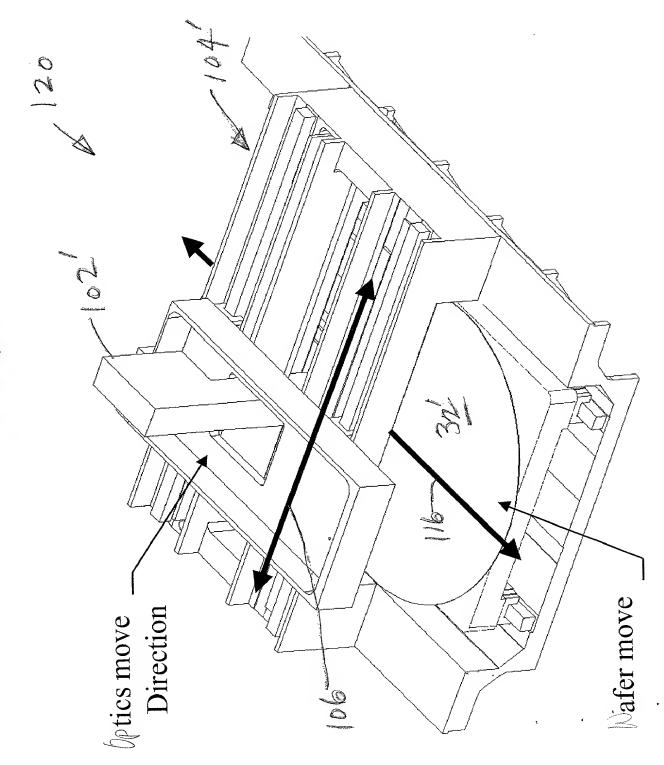

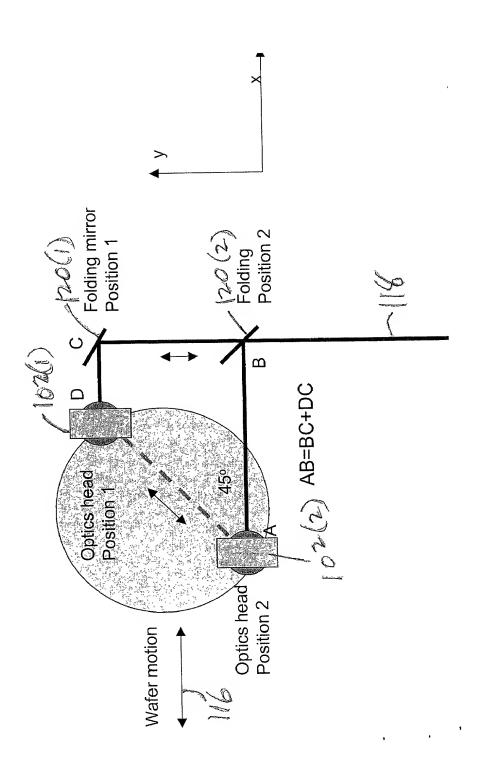

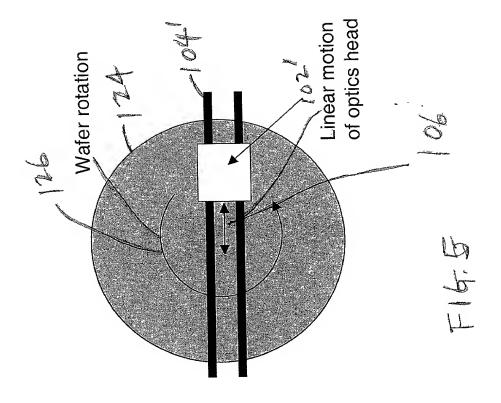
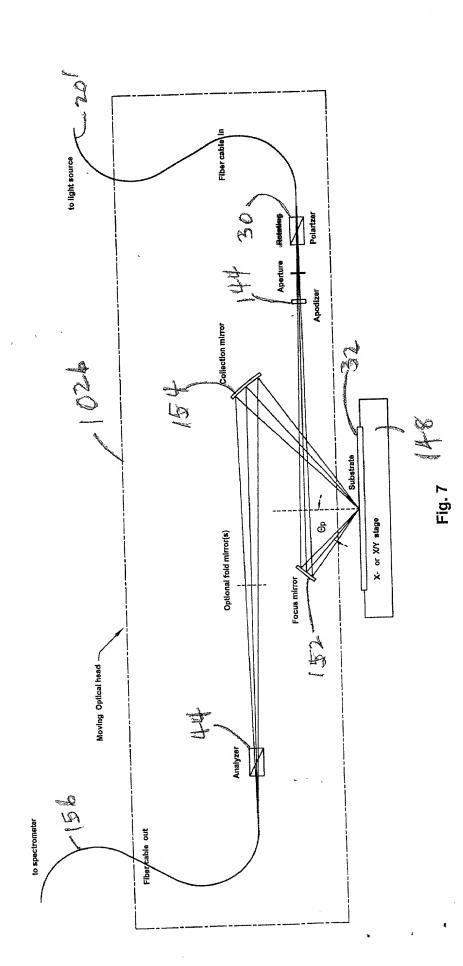


Fig. 6





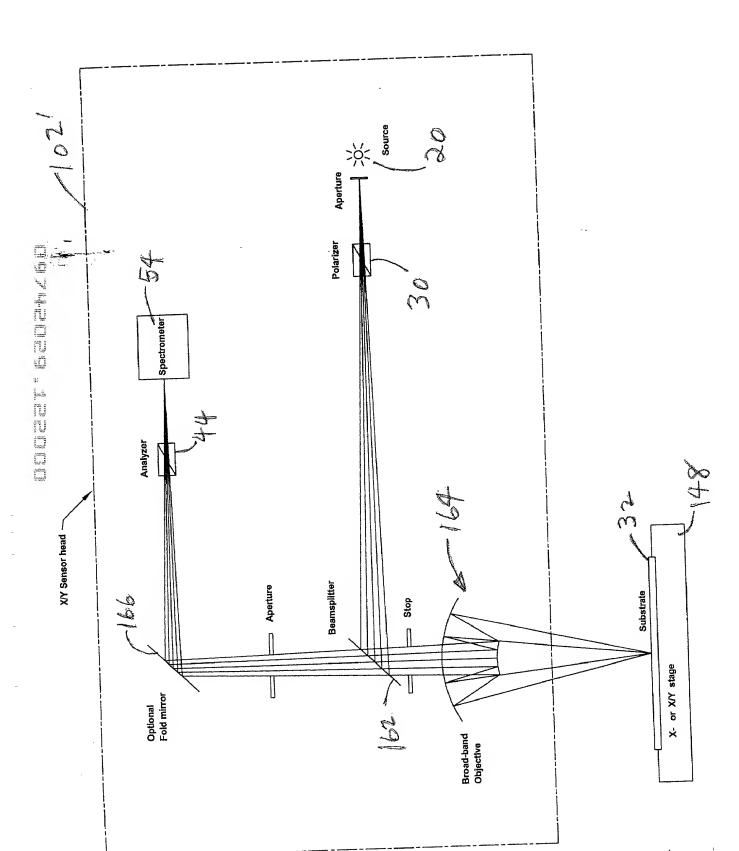


Fig.




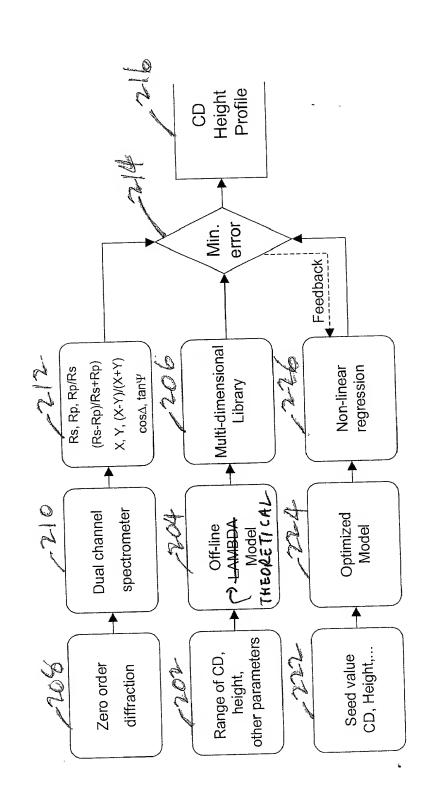

F14. # 10

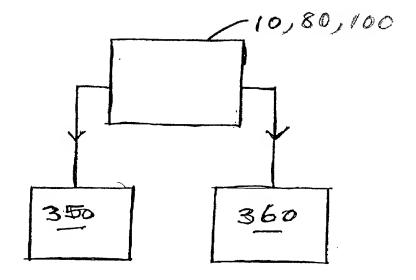

Points of Integration

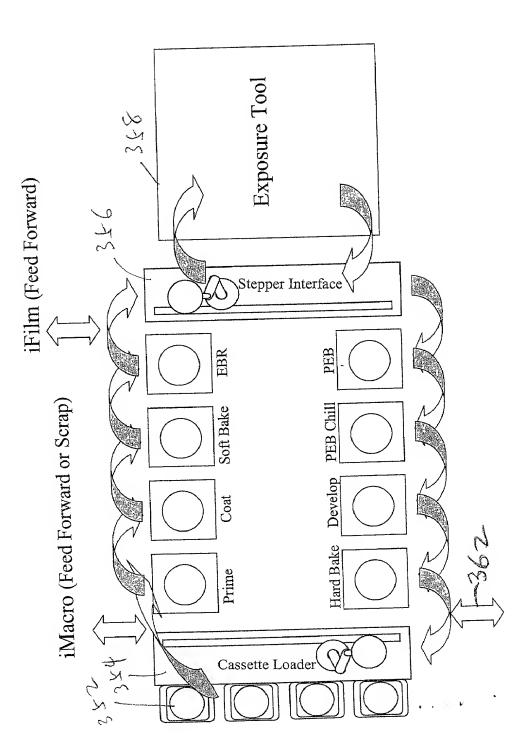

iCD (Feed Forward/Back)